



Australian Government

Department of Industry,
Science and Resources

**National
Measurement
Institute**

36 Bradfield Road, West Lindfield NSW 2070

Supplementary Certificate of Approval

NMI S861

Issued by the Chief Metrologist under Regulation 60
of the
National Measurement Regulations 1999

This is to certify that an approval for use for trade has been granted in respect of the instruments herein described.

Anyload Model 102BS Load Cell

submitted by Associated Scale Services Pty. Ltd.
Shop 4/47 Learoyd Road
Acacia Ridge QLD 4110

NOTE: This Certificate relates to the suitability of the pattern of the instrument for use for trade only in respect of its metrological characteristics. This Certificate does not constitute or imply any guarantee of compliance by the manufacturer or any other person with any requirements regarding safety.

This approval has been granted with reference to document NMI R 60, *Metrological Regulation for Load Cells*, dated July 2004.

This approval is subject to review at the decision of the Chief Metrologist in accordance with the conditions specified in the document NMI P 106.

DOCUMENT HISTORY

Rev	Reason/Details	Date
0	Pattern approved – certificate issued	04/09/24

CONDITIONS OF APPROVAL

General


Instruments purporting to comply with this approval shall be marked with approval number 'NMI S861' and only by persons authorised by the submitter.

Instruments incorporating a component purporting to comply with this approval shall be marked 'NMI S861' in addition to the approval number of the instrument, and only by persons authorised by the submitter.

It is the submitter's responsibility to ensure that all instruments marked with this approval number are constructed as described in the documentation lodged with the National Measurement Institute (NMI) and with the relevant Certificate of Approval and Technical Schedule. Failure to comply with this Condition may attract penalties under Section 19B of the National Measurement Act and may result in cancellation or withdrawal of the approval, in accordance with document NMI P 106.

The values of the performance criteria (maximum number of scale intervals etc.) applicable to an instrument incorporating the pattern approved herein shall be within the limits specified herein and in any approval documentation for the other components.

Signed by a person authorised by the Chief Metrologist to exercise their powers under Regulation 60 of the *National Measurement Regulations 1999*.

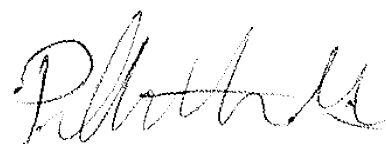

Phillip Mitchell
(A/g) Manager
Policy and Regulatory Services

TECHNICAL SCHEDULE No S861

1. Description of Pattern

approved on 04/09/24

An Anyload model 102BS stainless steel double ended shear beam load cell of 30 000 kg maximum capacity (Figure 1 and Table 1) and approved for use with up to 5 000 verification scale intervals.

1.1 Method of Mounting

Mounting is to be in accordance with the manufacturer’s instructions and as shown in Figure 2.

1.2 Markings

Each load cell is marked with the following:

Manufacturer’s mark, or name written in full	Anyload Younzon Transducer (Hangzhou) Co., Ltd.
Model number
Maximum capacity	E_{max} kg (or t)
Serial number
Pattern approval mark	NMI S861

1.3 Table of Specifications

Specifications for the pattern are given in Table 1.

TABLE 1

Model Number	102BS						
E_{max} (kg)	11 000	15 000	20 000	25 000	30 000	35 000	50 000
E_{min} (kg)	0						
Class	C						
nLC	5 000						
V_{min} (kg)	0.733	1.000	1.333	1.667	2.000	2.333	3.333
DR (kg)	1.100	1.500	2.000	2.500	3.000	3.500	5.000
mV/V	3						
Input imp (Ω)	750						
Voltage (V)	12						
Cable length (m)*	18.1						
Number of leads (plus shield)	4						

*Load cell cable shall not be altered after manufactured.

Where:

- E_{max} = Maximum capacity
- E_{min} = Minimum dead load
- nLC = Maximum number of verification intervals
- V_{min} = Minimum value of verification interval


DR	=	Minimum dead load output return value
mV/V	=	Output rating (nominal)
Input imp.	=	Input impedance (nominal)
Voltage	=	Maximum supply voltage (AC/DC)

FIGURE S861 – 1



Anyload Model 102BS Load Cell

FIGURE S861 – 2

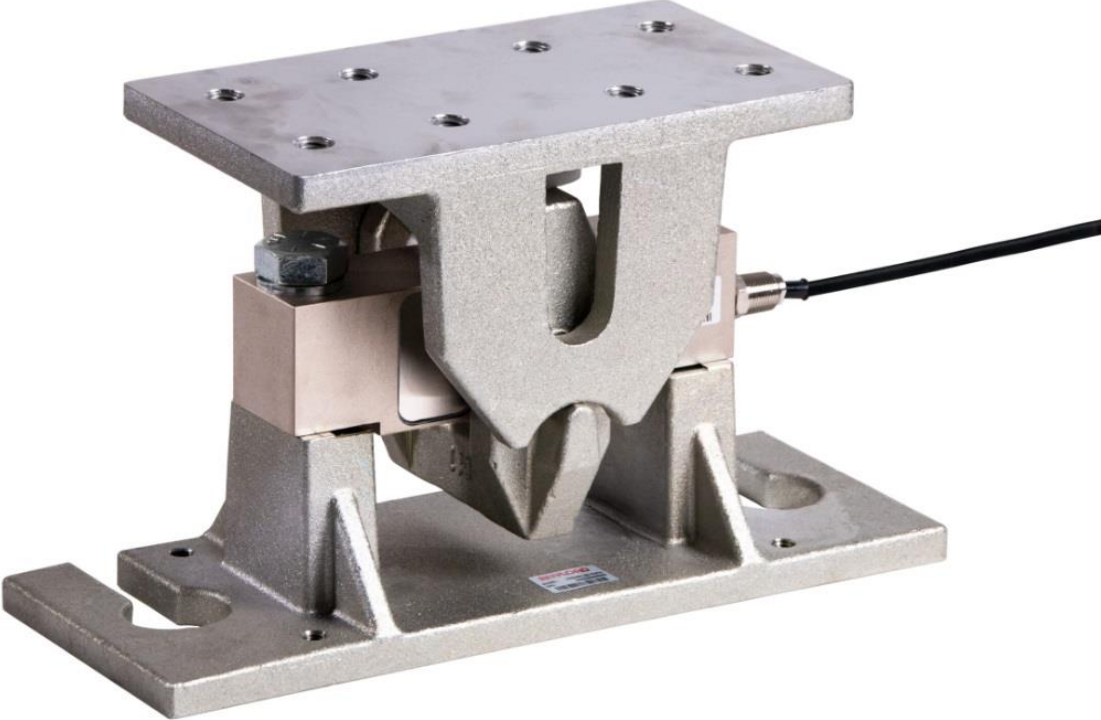

Typical Mounting Arrangement

~ End of Document ~