

6/3/4A
12/5/86



NATIONAL STANDARDS COMMISSION

NATIONAL MEASUREMENT (PATTERNS OF INSTRUMENTS) REGULATIONS

REGULATION 9

CERTIFICATE OF APPROVAL No 6/3/4A

This is to certify that an approval for use for trade has been granted in respect of the pattern and variant of the

Avery Model 2108 Weighing Instrument

submitted by Avery Australia Ltd
3-5 Birmingham Avenue
Villawood NSW 2163.

This Certificate is issued upon completion of a review of NSC Approval No 6/3/4.

Conditions of Approval

This approval is subject to review on or after 1/4/91.

Instruments purporting to comply with this approval shall be marked NSC No 6/3/4A. Instruments currently marked 6/3/4, and which comply with this approval, may be remarked 6/3/4A at their next verification.

This approval may be withdrawn if instruments are constructed and used other than in accordance with the drawings and specifications lodged with the Commission.

Signed

Executive Director

Descriptive Advice

Pattern: approved 20/3/86

- . A non-self-indicating weighing instrument of 15 kg capacity with a verification scale interval of 0.010 kg.

Variant: approved 20/3/86

1. Other capacities as listed in Table 1.

Technical Schedule No 6/3/4A describes the pattern and variant.

Filing Advice

The documentation for this approval comprises:

- Certificate of Approval No 6/3/4A dated 12/5/86
- Technical Schedule No 6/3/4A dated 12/5/86 (including Table 1)
- Test Procedure No 6/3/4A dated 12/5/86
- Figure 1 dated 12/5/86



NATIONAL STANDARDS COMMISSION

TECHNICAL SCHEDULE No 6/3/4A

Pattern: Avery Model 2108 Weighing Instrument

Submittor: Avery Australia Ltd
3-5 Birmingham Avenue
Villawood NSW 2163

1. Description of Pattern

A non-self-indicating weighing instrument of 15 kg capacity with a verification scale interval of 0,010 kg (Figure 1 and Table 1). The mass receptor and load receptor are located above the equal-arm beam and are maintained horizontal by a Roberval lever mechanism.

1.1 Zero Setting

The instrument is provided with a balance indicator and a balancing chamber is located beneath the load receptor.

1.2 Markings

The instrument is marked with the following data, together in one location:

Manufacturer's name or mark	
Serial number	
NSC approval number	NSC No 6/3/4A
Accuracy class	III
Maximum capacity	Max kg
Minimum capacity	Min kg
Verification scale interval	e = kg

1.3 Verification Provision

Provision is made for a verification mark to be applied.

2. Description of Variant 1

Other capacities as listed in Table 1.

TABLE 1

Maximum Capacity	Minimum Capacity	Verification Scale Interval (e)
10 kg	0,250 kg	0,005 kg
15 kg	0,375 kg	0,010 kg
25 kg	0,625 kg	0,010 kg

TEST PROCEDURE No 6/3/4A

The maximum permissible errors are:

- ± 0,5e for loads between 0 and 500e;
- ± 1,0e for loads between 501e and 2000e; and
- ± 1,5e for loads above 2000e.

1. Zero Test

With no load on either receptor of the instrument, it should be readily discernable that the instrument is at zero, by the alignment of the indexes.

2. Load Test

Test loads are to be applied to the instrument in not less than 5 approximately equal steps increasing to maximum capacity, followed by decreasing loads in not less than 5 approximately equal steps to zero load.


3. Sensitivity Test at Initial Verification

A mass equal to the verification scale interval placed on or subtracted from the instrument at equilibrium, loaded or unloaded, shall cause the indicating element to move to, but not necessarily remain at the limit of its movement.

4. Off-centre Load Test

The instrument should satisfy the maximum permissible errors above when a load corresponding to 1/3 maximum capacity is distributed successively along each edge of the load or weights receptor without excessive stacking or overlapping of the edges.

FIGURE 6/3/4A - 1

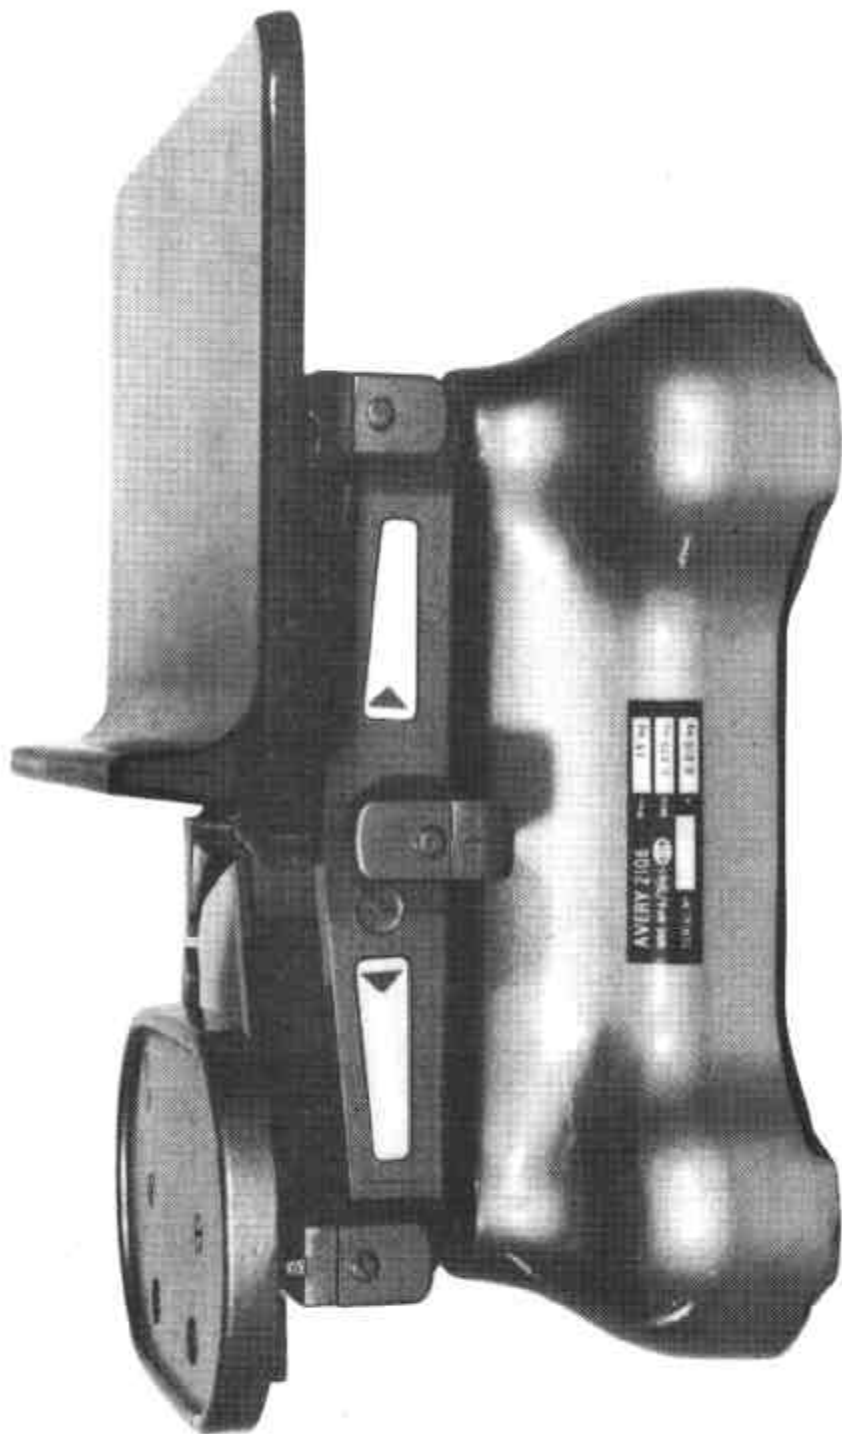

Avery Model 210B