

Australian Government Department of Industry, Innovation and Science

National Measurement Institute

# **Supplementary Certificate of Approval**

# **NMI S428**

Issued by the Chief Metrologist under Regulation 60 of the National Measurement Regulations 1999

This is to certify that an approval for use for trade has been granted in respect of the instruments herein described.

Mettler Toledo (Changzchou) Model SBH-2 Load Cell

submitted by	Mettler Toledo Lim	ited	
	220 Turner Street		
	Port Melbourne	VIC	3207

**NOTE:** This Certificate relates to the suitability of the pattern of the instrument for use for trade only in respect of its metrological characteristics. This Certificate does not constitute or imply any guarantee of compliance by the manufacturer or any other person with any requirements regarding safety.

This approval has been granted with reference to document NMI R 60, *Metrological Regulation for Load Cells*, dated July 2004.

This approval becomes subject to review on 1/02/21, and then every 5 years thereafter.

Rev	Reason/Details	Date
0	Pattern and variant 1 approved – interim certificate issued	28/01/04
1	Pattern and variant 1 approved – certificate issued	25/05/04
2	Pattern and variant 1 reviewed – notification of change issued	30/07/09
3	Pattern and variant 1 reviewed, amended (Figure 3 added) &	9/06/16
	updated – certificate issued	

DOCUMENT HISTORY

# CONDITIONS OF APPROVAL

#### General

Instruments purporting to comply with this approval shall be marked with approval number 'NMI S428' and only by persons authorised by the submittor.

Instruments incorporating a component purporting to comply with this approval shall be marked 'NMI S428' in addition to the approval number of the instrument, and only by persons authorised by the submittor.

It is the submittor's responsibility to ensure that all instruments marked with this approval number are constructed as described in the documentation lodged with the National Measurement Institute (NMI) and with the relevant Certificate of Approval and Technical Schedule. Failure to comply with this Condition may attract penalties under Section 19B of the National Measurement Act and may result in cancellation or withdrawal of the approval, in accordance with document NMI P 106.

The values of the performance criteria (maximum number of scale intervals etc.) applicable to an instrument incorporating the pattern approved herein shall be within the limits specified herein and in any approval documentation for the other components.

Signed by a person authorised by the Chief Metrologist to exercise their powers under Regulation 60 of the *National Measurement Regulations 1999*.

Dr A Rawlinson

# TECHNICAL SCHEDULE No S428

#### 1. Description of Pattern

A Mettler-Toledo (Changzchou) model SBH-2 load cell of 2000 kg maximum capacity (Figure 1 and Table 1) approved for use with up to 3000 verification intervals.

#### 1.1 Method of Mounting

Mounting is to be in accordance with the manufacturer's instructions and as shown in Figures 2 or 3.

Note: Load cells may also be provided with holes adjacent to the loading point of the load cell, intended for a clip to retain a loading foot or similar.

#### 1.2 Markings

Each load cell is marked with the following:

Manufacturer's mark, or name written in full

Mettler-Toledo (Changzchou) Scale & Systems Ltd

..... kg

**NMI S428** 

....

approved on 28/01/04

Model number Maximum capacity, *E<sub>max</sub>* Serial number Pattern approval mark

# **1.3 Table of Specifications**

Specifications for the pattern are given in Table 1.

#### 2. Description of Variant 1

approved on 28/01/04


Certain other capacities of the SBH series as listed in Table 1.

TABLE	1
-------	---

Type: Mettler-Toledo (Changzchou) SBH Series

Model number:	SBH-0.25	SBH-0.5	SBH-1	SBH-2
Maximum capacity, <i>E<sub>max</sub></i> (kg)	250	500	1000	2000
Accuracy class	С	С	С	С
Maximum number of verification intervals, nLC	3000	3000	3000	3000
Minimum value of verification interval, <i>v<sub>min</sub></i> (kg)	0.04	0.08	0.17	0.33
Minimum dead load output return value, DR (kg)	0.015	0.03	0.06	0.12
Output rating (nominal), mV/V	2	2	2	2
Input impedance (nominal), $(\Omega)$	350	350	350	350
Supply voltage (Max, AC or DC), (V)	20	20	20	20
Cable length (±0.1 m), (m)	3	3	3	3
Number of leads (plus shield)	4	4	4	4


FIGURE S428 - 1

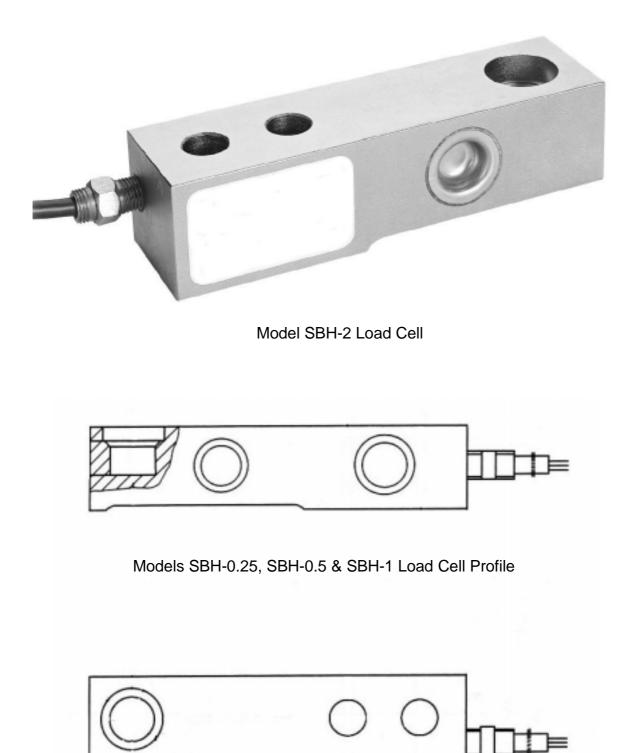

Typical Mettler-Toledo (Changzchou) SBH Series Load Cells

Page 5 of 5

FIGURE S428 - 2

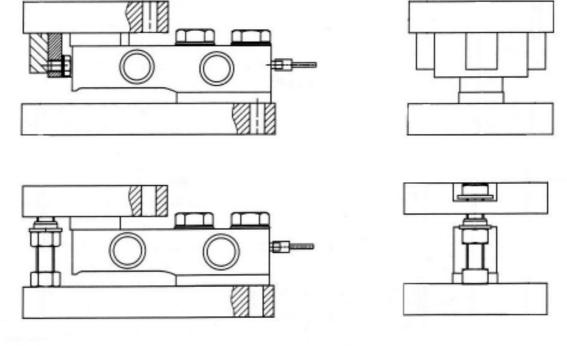

Mettler-Toledo (Changzchou) SBH Series Load Cells - Alternative Mounting Methods

FIGURE S428 - 3

Alternative Mounting Method ('MultiMount')

~ End of Document ~

